


# REICHERT SPR SYSTEMS

## APPLICATION NOTE 12

# Reichert SPR Phage-Antibody Selection using a Reichert SPR Instrument

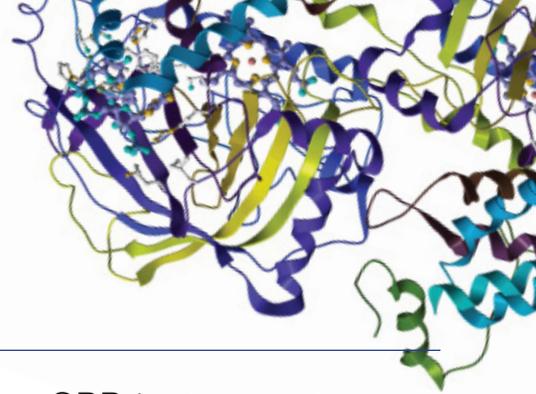

This preliminary note involves the novel use of a Reichert SPR instrument to perform enrichment of phage antibodies using the fluidics system of the instrument. Phage antibody technology is a powerful method for obtaining specific antibodies directed at a defined target for a fraction of the time and cost of conventional monoclonal antibody technology. It was theorized that if phage encoding a binding partner for a target immobilized on a sensor slide could be separated from phage displaying non-binding proteins, then it would be possible to employ the precise fluidic controls of the instrument to perform enrichments under conditions that could prove beneficial in selecting affinity variants.

### Experimental

The Reichert SPR instrument was used with a Reichert planar mixed SAM sensor chip and PBST as the running buffer. Approximately 1500  $\mu$ RIU of BSA was amine-coupled to the left channel only of a two channel instrument. Phage displaying either an anti-BSA antibody (single-chain Fc, scFv) or an anti-peptide scFv (negative control) that can be easily distinguished by a colony PCR procedure were prepared and injected onto the sensor chip. Phage were applied at a flow rate of 10  $\mu$ l/min. After 10 minutes, the flow rate was increased to 50  $\mu$ l/min and aliquots of the out-flow were collected. After approximately 20 minutes of dissociation, remaining sample was eluted by injection of 20 mM HCl and additional fractions collected. Phages present in the fractions were recovered by transduction of E. coli and samples of colonies in each fraction were subjected to colony PCR. The products were resolved by agarose gel electrophoresis.

### Results

A summary of SPR and fractionation results are presented in Figures 1-3.

A total of about  $1 \times 10^8$  to the 8th power phage consisting of roughly equal amounts of a BSA binder and a non-binding anti-peptide phage were injected. The delta SPR signal from the injection is shown here. After phage is flowed over the BSA target and dissociated, the material remaining bound material on the surface is removed by regeneration with 20 mM HCl. Anti-BSA Mab is then injected as a control to show the surface is still active. After dissociation, the surface is again regenerated with 20 mM HCl.

Pictorial with timing of the separation of BSA binder and non-binder phage. Amounts of phage found in each titer of fractions is shown. Recovery is 1-5% when applying  $\sim 1 \times 10^8$  to the 8th power binding phage. Upper values at the bottom are for phage that bound, lower values are for negative control (these numbers indicate good specificity). Results clearly show a 10 to the 3rd power enrichment...with a non-optimized system.

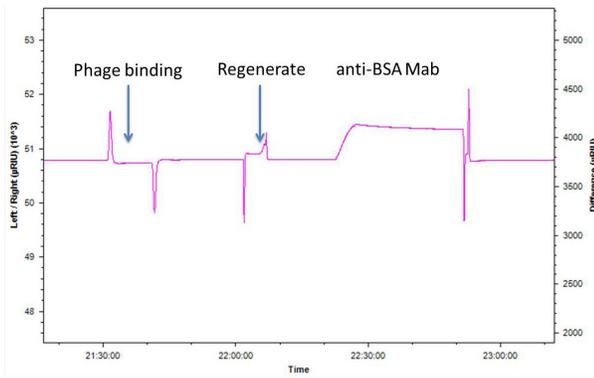


Figure 1

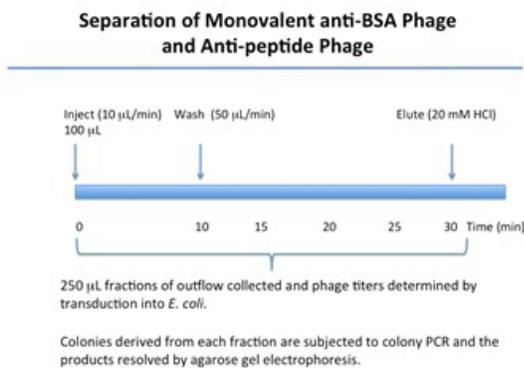


Figure 2

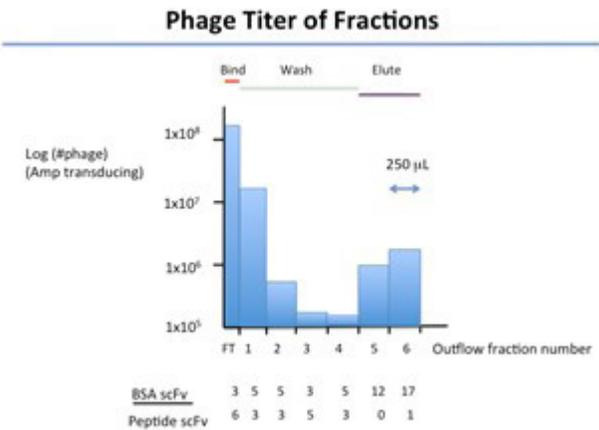


Figure 3

### Conclusions

Preliminary results indicate that phage can be easily applied, fractionated and recovered from the SPR outflow after elution.

1. Binding phage can be readily separated from non-binders using SPR. Results clearly show a 103 enrichment even though the system is not optimized.
2. The SPR signal may be useful in characterization of panels of similar clones with varying affinities. It will be essential to use only monovalent phage. The yield of phage seems to be dependent on the target levels immobilized and affinity.
3. Increasing the number of displaying phage in the input is desirable. The SPR signal is unlikely to be helpful when enriching for low abundance binders.

### Potential Opportunities/Future Directions

1. Use SPR to characterize individual phage binding kinetics and to rank affinities.
2. Do binder selection using SPR affinity in phage. This would allow protein expression to be skipped.
3. Use elution control to eliminate low affinity binders and improve reproducibility. Vary parameters such as flow rate, temperature, time, concentration and elution buffer composition depending on the relative affinities of the population.
4. Immobilize different targets on different channels - this would allow for customization of specificity. Since there are multiple channels on the SPR, multiple enrichments could be run simultaneously

---

**Learn more about how Reichert pushes the limits of detection and sensitivity in label-free interaction. To improve the quality of your protein interaction research, visit [www.ReichertSPR.com](http://www.ReichertSPR.com)**

---

®\*Trademark of Reichert Technologies Company Notice: No freedom from infringement of any patent owned by Reichert or others is to be inferred. Because use conditions and applicable laws may differ from one location to another and may change with time, Customer is responsible for determining whether products and the information in this document are appropriate for Customer's use and for ensuring that Customer's workplace and disposal practices are in compliance with applicable laws and other government enactments. The product shown in this literature may not be available for sale and/or available in all geographies where Reichert is represented. The claims made may not have been approved for use in all countries. Reichert assumes no obligation or liability for the information in this document. References to "Reichert" or the "Company" mean the Reichert legal entity selling the products to Customer unless otherwise expressly noted. NO WARRANTIES ARE GIVEN; ALL IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE ARE EXPRESSLY EXCLUDED.

**Corporate Office**  
Reichert Technologies  
3362 Walden Avenue  
Buffalo, New York 14043, USA  
Tel: +1 716-686-4500  
Fax: +1 716-686-4555  
Toll Free USA: 1-888-849-8955  
[reichertspr.lifesciences@ametek.com](mailto:reichertspr.lifesciences@ametek.com)

**European Service Center**  
Carl-von-Linde Str. 42-85716  
Unterschleissheim/Munich, Germany  
Tel: +49 89 315 8911 0  
Fax: +49 89 315 891

[www.reichertspr.com](http://www.reichertspr.com)